

Operations Manual

Item: C1008

V1.0

myFUGE™ Mini



Introduction:

Thank you for purchasing the **MyFuge™** Mini Centrifuge. Please read this manual thoroughly prior to operating the instrument.

The **MyFuge** Mini Centrifuge is designed for low speed applications and quick spin downs of microcentrifuge tubes (0.2ml - 2.0ml) and for eight position PCR strips.

Specifications:

Speed: 6000 rpm / 2000xg
Capacity: 8 x 1.5/2.0ml
16 x 0.2ml or 2 x PCR strips
Dimensions: 4.5 (W) x 5.9 (D) x 4.5 (H) in.
11.4 (W) x 15 (D) x 11.4(H) cm
Electrical: 120V to 240V, 50-60 Hz
Max. Radius: 4.9cm

Installation:

Place the **MyFuge** mini-centrifuge on a flat and level surface nearby an electrical outlet. It should not be near a heat source or in direct sunlight.

Rotor Exchange:

The **MyFuge** mini-centrifuge includes a second rotor that is designed for holding PCR tubes (0.2ml) and PCR strips (8 position). The rotor is conveniently stored in a compartment on the bottom of the centrifuge. To access this rotor, turn the machine upside down and remove it from the compartment.


- Removing the Rotor from the motor shaft:

Use the included allen key to loosen the set screw located on the bottom of the rotor by turning counter-clockwise 4-5 complete turns. The rotor can now be removed by lifting it evenly off of the rotor shaft.

- Attaching the Rotor to the motor shaft:

Place the rotor on the motor shaft and press down until the rotor comes to a stop. The set screw can now be tightened by inserting the allen key and turning clockwise 4-5 complete turns.

Operation:


- Attach the power cord and place the power switch into the on “-” position.
 - Open the lid and load your samples into the rotor. Always ensure a balanced load (Please see the following section, **Loading the Rotor**, for details.)
 - Close the lid, the rotor quickly accelerates to the maximum speed of 6200 rpm.
 - When the desired run time is completed, push on the lid button to open the lid, the rotor quickly brakes to a stop and the samples can be retrieved.
-  NEVER Attempt: to remove samples until the rotor has come to a complete stop.

Loading the Rotor:

To ensure safe operation and long life of the instrument, samples must always be loaded into the rotor in a balanced fashion.

Tubes and strips must always be loaded symmetrically across from one another and contain the same volume of liquid. See below:


Examples of properly balanced rotors:

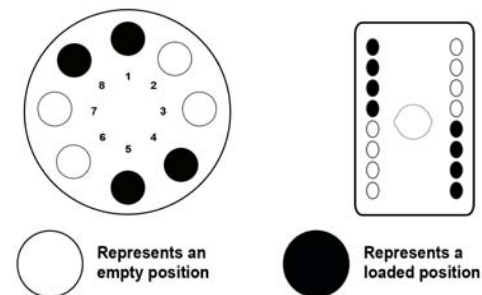

 Represents an empty position

 Represents a loaded position

Examples of improperly balanced rotors:

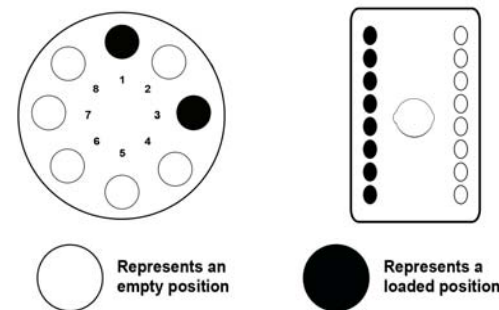

 Represents an empty position

 Represents a loaded position

Cleaning and Maintenance:

The centrifuge rotors can be removed for cleaning by using the included allen wrench to loosen the set screw. Once removed, the rotors can be cleaned with isopropyl alcohol or can be sterilized in an autoclave at 121°C for 20 minutes.

Service and Contact:

In the event that service or technical support is required, please contact **Benchmark** by phone at **1-908-769-5555**.

American MasterTech
scientific laboratory supplies

1330 Thurman Street
Lodi, CA 95240

Phone: 800.860.4073
Fax: 209.368.4136

www.americanmastertech.com